




『 **CERTIFICATE OF ANALYSIS** 』

Fullerene C60 chromatogram

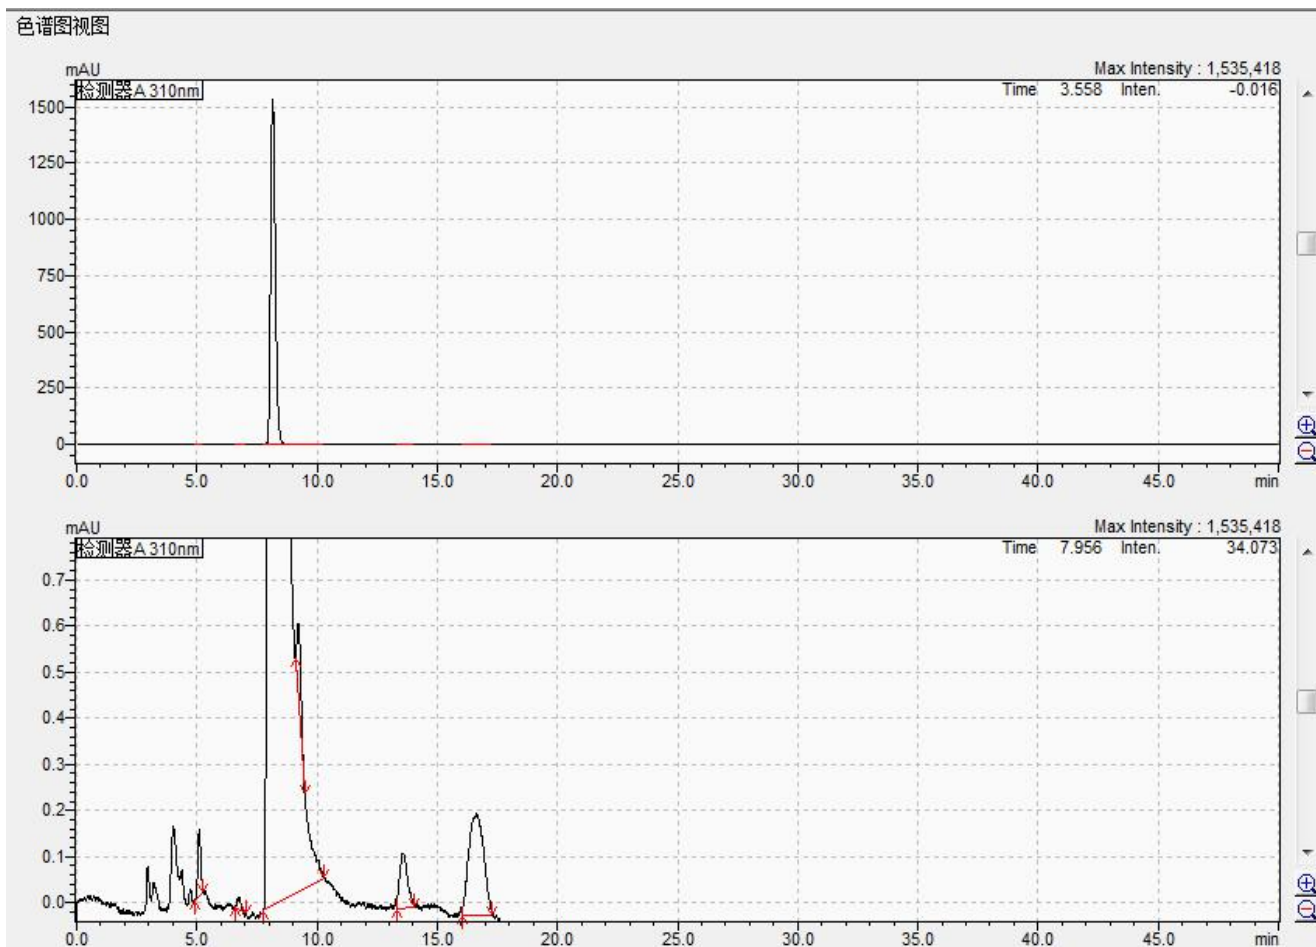

Fullerene C60 Purity Test Results:99.924%

Items	Retention Time	Area	Peak Time	Start Time	Peak Time	End	Area(%)	Remark
1	5.103	1254	4.925	5.250			0.006	
2	6.709	254	6.600	7.050			0.001	
3	8.155	20750871	7.758	10.300			99.924	C60
4	9.214	2087	9.092	9.483			0.010	C60 Oxides
5	13.567	2729	13.333	14.033			0.013	C70
6	16.642	9520	16.067	17.283			0.046	
Total		20766715	4.925				100.000	

Analyst:Shiluping

Checker:Yangjiping



Q.C Director: Dinglicha