

Non-ophthalmic institutions can also easily operation Reduce the workload of the operator

LEARNING PROCESS

Visually display patient instruction to make the test faster, easier and more reliable.

VOICE PROMPT

System voice prompt to reduce mechanical workload, save time for operator.


DICOM


Easy communication and more convenient upload and download of customer's information.

BINOCULAR REPORT(2 IN 1)

Right and left eye test result in one report, paper-saved and environmental friendly.

Especially suitable for comprehensive physical examination.

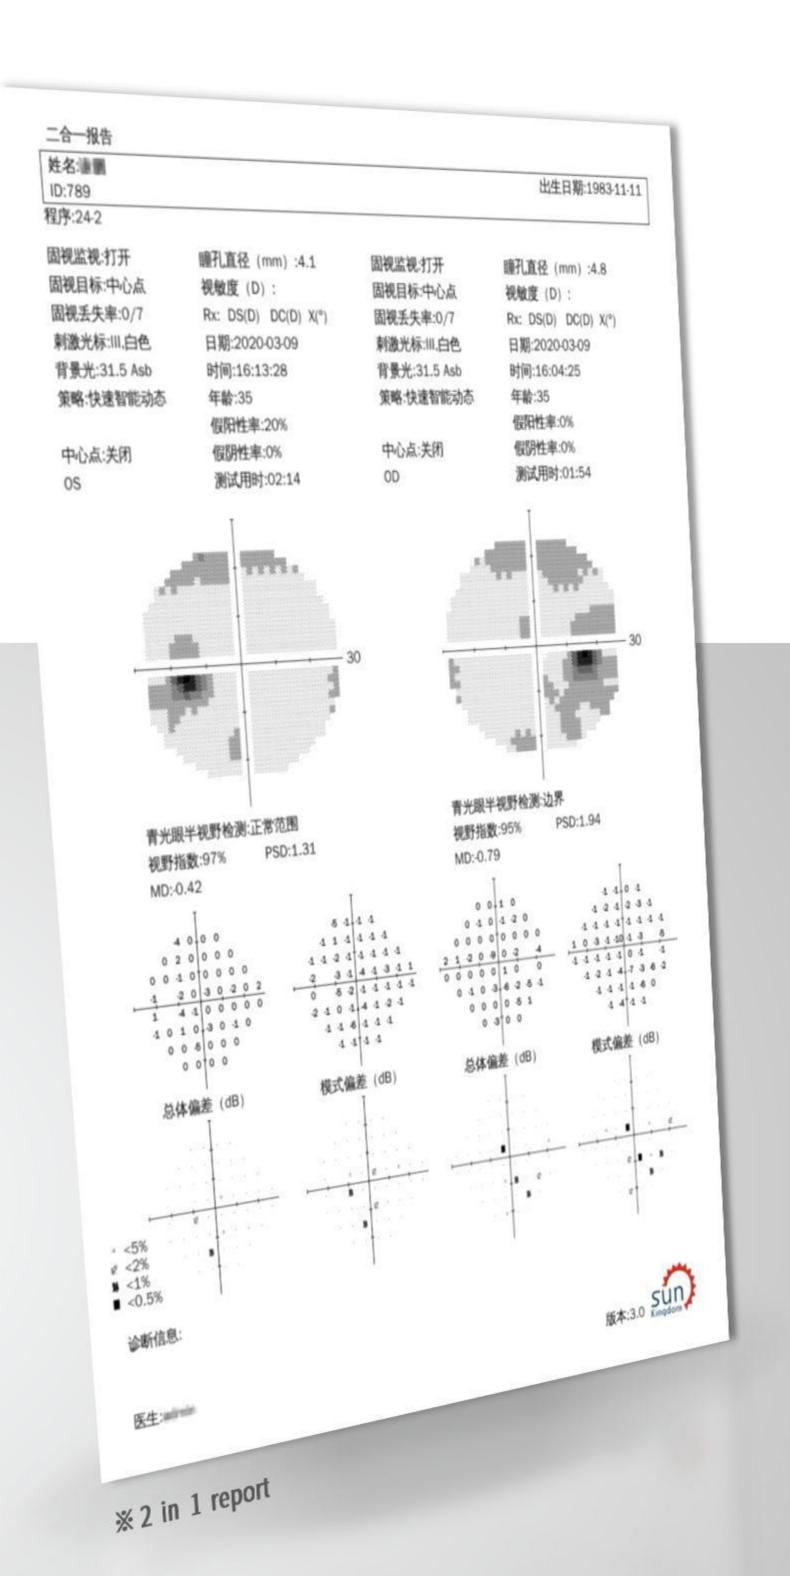

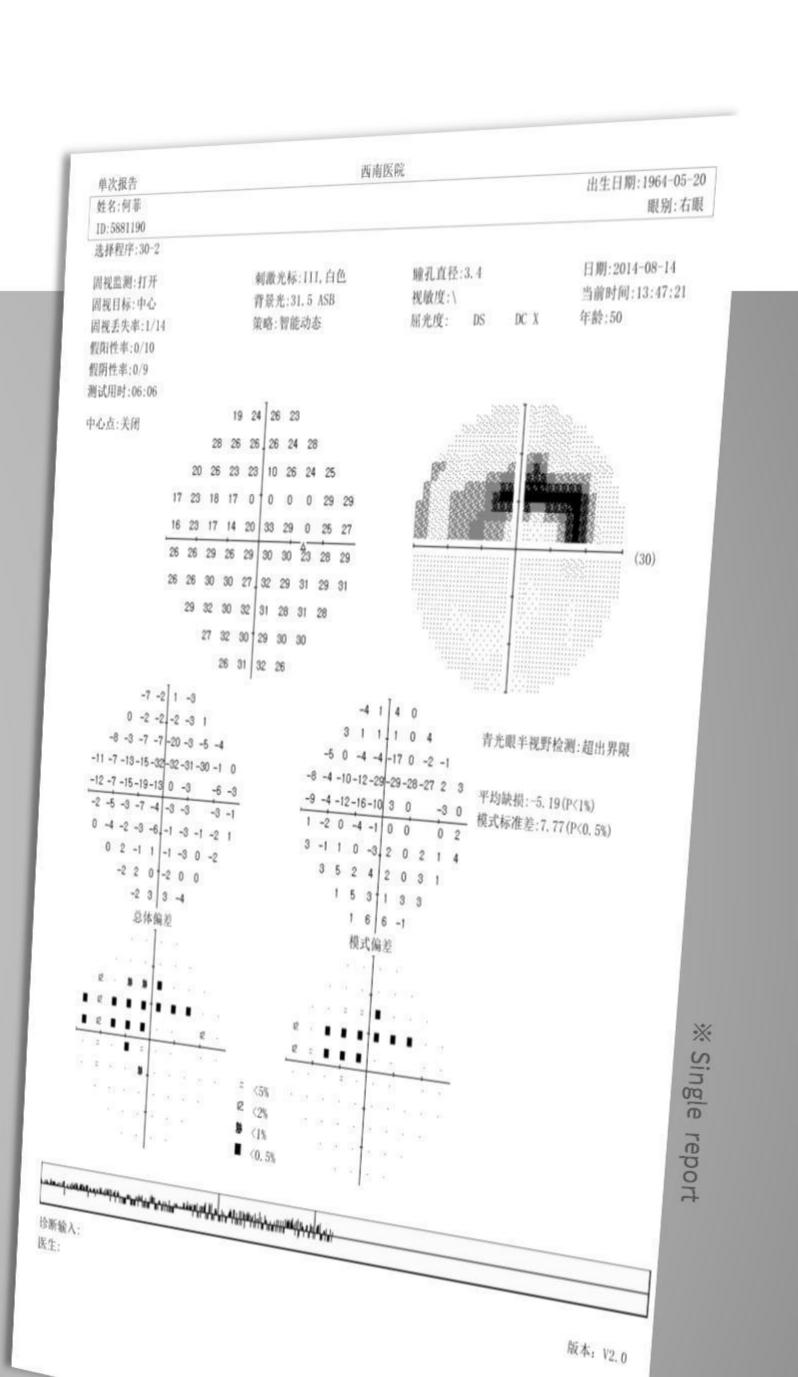

TECHNICAL PARAMETER

| | SK-850B | SK-850C | SK-950B | SK-950C |
|-----------------------------|---|------------------------------|---------------------------|------------------------------|
| Projective plane | Aspherical surface | | | |
| Max measurement range | 90° | | | |
| Testing distance | 300mm | | | |
| DB value range | 0-51db | | | |
| Calibration | Self checking | Self checking | Self checking with report | Self checking with repor |
| System | windos | windos | Embedded Linux | Embedded Linux |
| DICOM | / | / | • | |
| Touch screen | Resistance type | Resistance type | Capacitive type | Capacitive type |
| Light source | Halogen | Halogen | LED | LED |
| Stimulus brightness control | Change optical progressive lens to control projection brightness | | | |
| Stimulus color control | Use optical filter to change projection color | | | |
| Stimulus color | White | White / Red / Blue | White | White / Red / Blue |
| Stimulus size | Goldmann III | Goldmann I-V | Goldmann I-V | Goldmann I-V |
| Background illu. | White31.5ASB | White31.5ASB Yellow315ASB | White31.5ASB | White31.5ASB Yellow315ASB |
| Auto pupil measurement | • | • | • | • |
| Fixation monitoring | Heijl/krakau blind spot monitor、 Video eye monitor、 Gaze tracking、 Head tracking、 Vertex monitor、 Gaze curve | | | |
| Auto-Chinrest tracking | • | • | • | |
| Voice prompt | / | / | • | • |
| Learning procedure | | / | • | • |
| Static test | • | • | • | • |
| Custom static test | • | • | • | • |
| Kinetic test | / | • | / | • |
| Custom kinetic test | 1 | • | / | • |
| SWAP | / | • | / | • |
| Eye playback | / | / | / | |
| Retest of doubts | / | / | • | • |
| GPA analysis | • | • | • | • |
| Binocular report | | | • | • |

OPTICAL KINETIC PERIMETER

SK-850B / SK-850C / SK-950B / SK-950C



STANDARD

Pure optical design, focus on every details Ensure every spot up to the standard





COMPREHENSIVE

Support static, screening, kinetic, special and custom programs Meet the needs of clinical and physical examination




ACCURATE AND RAPID

Different age, response ability, visual field defect and island distribution were considered in the design of examination strategy.


The detection time is faster and the clinical result is more accurate.



Pure optical design, focus on every details Ensure every spot up to the standard

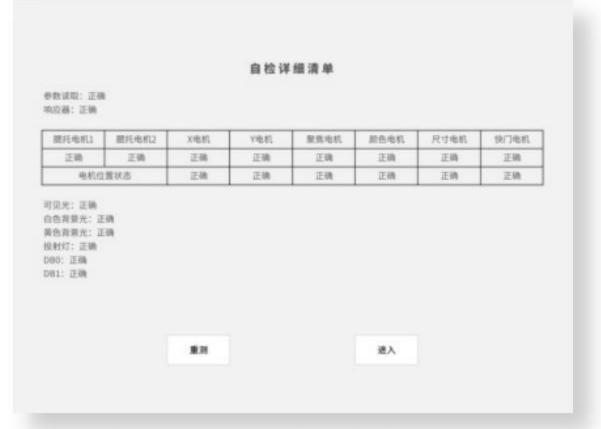

Detailed self-checking list

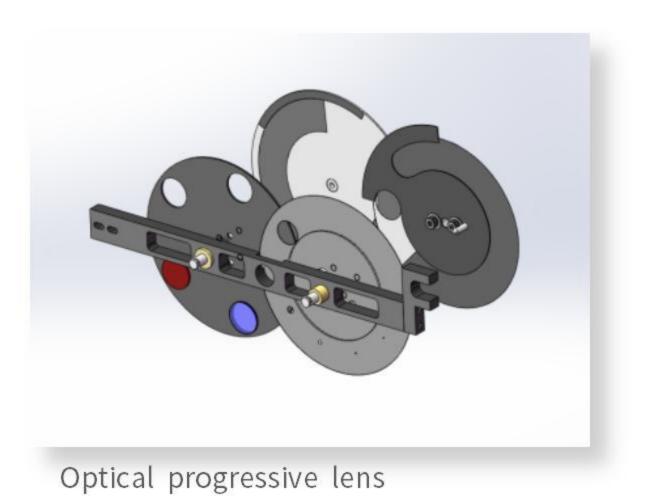

SELF-CHECKING DESIGN

Auto self-checking when powered on
Real time display self checking procedure
Detailed checking list presented
Easily obtain the perimeter current status

LED LIGHT SOURCE

Perfectly adopted LED as light source according to standard Longer life time, more stable No need regular lamp replace

PURE OPTICAL CONTROL

Coated progressive lens to control the light intencity and color Make sure the color temprature up to standard



BLUE-ON-YELLOW DETECTION

The light spot and background light of standard color temperature can be obtained through optical lens, which can stimulate blue cone cells accurately and help doctors to screen early glaucoma.





Improve the overall monitoring design, objectively feedback the cooperation of the examinee and ensure report reliability

EYE PLAYBACK

Trace for every dots fixation status avoid misdiagnose.

RETEST OF DOUBTS

Select several test points to retest, verify the reliability results, save the recheck time.

MONITORING SYSTEM

3D monitoring, infrared light on trial lens ensure the sensitivity and accuracy of eye position

Blind spot detection, eye tracking, head tracking and other monitoring procedures reduce the detection error caused by cooperative factors, provide objective feedback on the reliability report.



Infrared projection trial lens holder